

**PCC #:** \_\_\_\_\_

**BILL TO:** \_\_\_\_\_

**ADDRESS:** \_\_\_\_\_

**SHIP TO:**  SAME AS BILLING \_\_\_\_\_

**ADDRESS:** \_\_\_\_\_

**SHIPPING:**  GROUND (FXGD)  STANDARD 2 DAY (FX2D)

**OVERNIGHT:**  PRIORITY (FX1D)  1st OVERNIGHT (FX1A)

OTHER: \_\_\_\_\_

**CLINICIAN:** \_\_\_\_\_

**CELL #:** \_\_\_\_\_

**PATIENT ID:** \_\_\_\_\_

**HEIGHT:** \_\_\_\_\_ **WEIGHT:** \_\_\_\_\_ **AGE:** \_\_\_\_\_

MALE  FEMALE

LEFT  RIGHT  BILATERAL

**OPS INVOICE/NG ENCOUNTER:** \_\_\_\_\_

**MEASUREMENT DATE:** \_\_\_\_\_

**IN-OFFICE REQUEST DATE & TIME:** \_\_\_\_\_

PROJECT NEWTON (Credit applied on prior auth. denial, details on One Hanger)

**HFN:**  PHOENIX  ORLANDO  KANSAS  CHICAGO  OTHER \_\_\_\_\_

**MEASUREMENTS (REQUIRED)**

**DESIRED BRIM STYLE** \*Suction (Seal-In) Available


2020 Carroll Quad  2020 ComfortFlex\*  2020 ComfortFlex Mature\*

2020 IPOC IC\*  2020 Narrow ML\*  2020 Soft Quad\*  CNC

Mild IPOS IC\*  Modified Quad  Other Brim: \_\_\_\_\_

Suction (Seal-In) Design (Check if Ordering)

Zero Reference Point -  Perineum†  Ischium **†Perineum must be used for all 2020 brimstyles**  
Measurements taken in  CM  IN

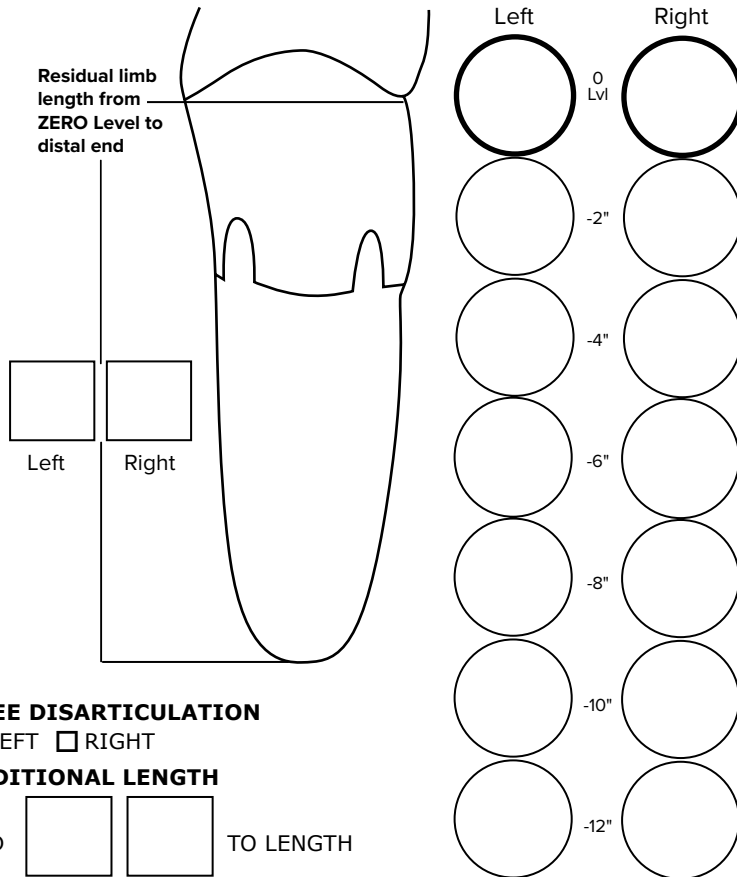

**KNEE DISARTICULATION**

LEFT  RIGHT

**ADDITIONAL LENGTH**

ADD   TO LENGTH  
Left Right

**ALIGNMENT**

FLEXION \_\_\_\_\_ ADDUCTION \_\_\_\_\_ ABDUCTION \_\_\_\_\_

**DESIGN**

**SCAN TYPE**

Already Modified by Clinician

Use Previous Model

Provide Date or CDC Order# \_\_\_\_\_

By Measurement Only

**Merge Order Scan Type**

Patient Scan  Positive Model Scan

**LINER SCANNED/MEASURED OVER**

Skin  Other: \_\_\_\_\_

**REDUCTION%**

0  1  2  3  4  5  6  7  8

CDC Reduction (Based on Liner/Tissue Type)

**TISSUE TYPE**

Firm  Medium  Soft

**DEVICE TYPE**

Carving Only

File Conversion

Check Socket Only

Laminated Socket Only

Check Socket & Carving

Laminated Socket & Carving

**Definitive Order Form Included**  Yes  No

**MATERIAL TYPE**

Vivac  Durplex  Other: \_\_\_\_\_

**SHAPE DISTAL END TO ACCEPT**

Endolite

USMC

Otto Bock 4 Hole

Grace Plate/Seattle 4 Hole

Other: \_\_\_\_\_

**INSTALLS**

Valve Type: \_\_\_\_\_

Distal Attachment Type: \_\_\_\_\_

Shuttle Lock Type: \_\_\_\_\_

**TURNAROUND TIMES**

To review current projected turnaround times for fabrication sites visit the [Daily HFN Capacity Webpage](#).