

**PCC #:** \_\_\_\_\_

**BILL TO:** \_\_\_\_\_

**ADDRESS:** \_\_\_\_\_

**SHIP TO:**  SAME AS BILLING \_\_\_\_\_

**ADDRESS:** \_\_\_\_\_

**SHIPPING:**  GROUND (FXGD)  STANDARD 2 DAY (FX2D)

**OVERNIGHT:**  PRIORITY (FX1D)  1st OVERNIGHT (FX1A)

OTHER: \_\_\_\_\_

**CLINICIAN:** \_\_\_\_\_

**CELL #:** \_\_\_\_\_

**PATIENT ID:** \_\_\_\_\_

**HEIGHT:** \_\_\_\_\_ **WEIGHT:** \_\_\_\_\_ **AGE:** \_\_\_\_\_

MALE  FEMALE

**NG ENCOUNTER #:** \_\_\_\_\_

**MEASUREMENT DATE:** \_\_\_\_\_


**IN-OFFICE REQUEST DATE & TIME:** \_\_\_\_\_

PROJECT NEWTON (Credit applied on prior auth. denial, details on One Hanger)


**HFN:**  CHICAGO  HOUSTON  PHOENIX  \_\_\_\_\_

**MEASUREMENTS (REQUIRED)**

**CRITICAL TO QUALITY**

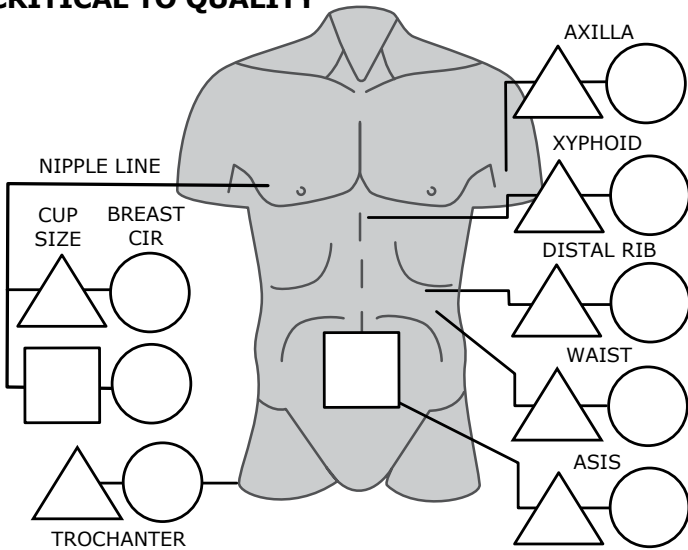

**ALL HEIGHT MEASUREMENTS TO BE TAKEN IN SUPINE**

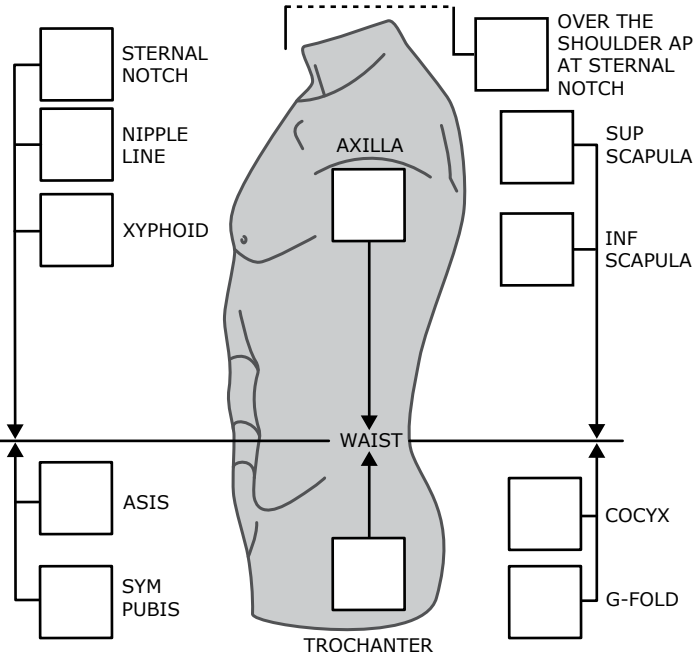

**DESIGN**

- Boston Style
- Boston Extreme
- Providence Style
- Nocturnal Pro (Formerly Prospine Night)
- Asymm/Goss Style
- Day Pro (Formerly Prospine Day)
- Nocturnal Bending Brace (Use NBB form)

**MEASUREMENT/INPUT [XRAY REQUIRED]**

- Supine
- Standing /
- Scan
- Cast

**CURVE TYPE APEX & MAGNITUDE**

- R  L Thoracic \_\_\_\_\_ Apex \_\_\_\_\_ Mag \_\_\_\_\_
- R  L Lumbar \_\_\_\_\_ Apex \_\_\_\_\_ Mag \_\_\_\_\_

**MODIFICATIONS**

- Lordosis  0°  10°  15°  20°  \_\_\_\_\_°
- Correction  Min  Standard  Aggressive
- ABD Relief  N/A  SM  MD  LG

Other Relief \_\_\_\_\_

**FINISH**

- Transfer  None Design \_\_\_\_\_
- Unfinished
- Vent Holes
- PE Tongue
- Pad Kit
- Compliance Monitor
- Outrigger
- Unlined
- Gusset
- Troch Extension
- Shoulder Strap
- Anterior Opening
- Other \_\_\_\_\_

**NOTES**

**TURNAROUND TIMES**

To review current projected turnaround times for fabrication sites visit the [Daily HFN Capacity Webpage](#).