

PCC #: \_\_\_\_\_

BILL TO: \_\_\_\_\_

ADDRESS: \_\_\_\_\_

SHIP TO:  SAME AS BILLING \_\_\_\_\_

ADDRESS: \_\_\_\_\_

SHIPPING:  GROUND (FXGD)  STANDARD 2 DAY (FX2D)  
OVERNIGHT:  PRIORITY (FX1D)  1st OVERNIGHT (FX1A)  
 OTHER: \_\_\_\_\_

CLINICIAN: \_\_\_\_\_

CELL #: \_\_\_\_\_

PATIENT ID: \_\_\_\_\_

HEIGHT: \_\_\_\_\_ WEIGHT: \_\_\_\_\_ AGE: \_\_\_\_\_

DIAGNOSIS: \_\_\_\_\_

**AFFECTED SIDE (Check One):**

LEFT  RIGHT or  BILATERAL: SYMMETRICAL  YES  NO

NG ENCOUNTER #: \_\_\_\_\_

MEASUREMENT DATE: \_\_\_\_\_

IN-OFFICE REQUEST DATE & TIME: \_\_\_\_\_


PROJECT NEWTON (Credit applied on prior auth. denial, details on One Hanger)

HFN:  KANSAS  ORLANDO  PHOENIX

If a Discrepancy Exists, Go By  Impression  Measurements **Units of Measure**  Millimeters  Inches


**PATIENT MEASUREMENTS (REQUIRED)**

PLEASE PROVIDE FINISHED HEIGHT/LENGTHS

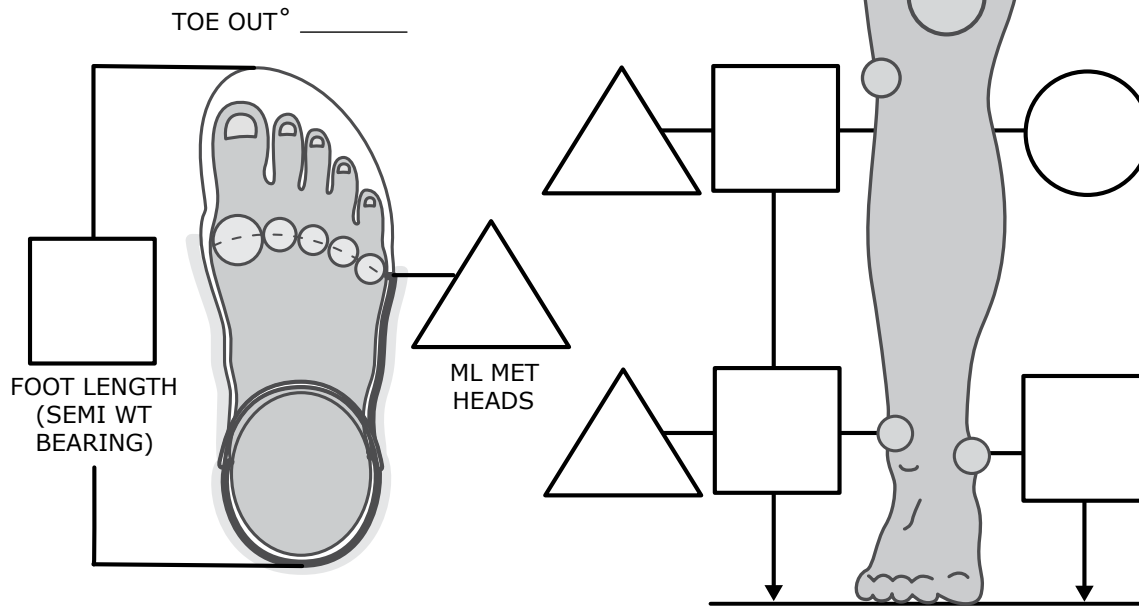

**TUNING CRITICAL MEASUREMENTS (Optional)**

Casting Block Used?  Yes\*  No \*Best Practice: Casting block improves design accuracy and efficiency.

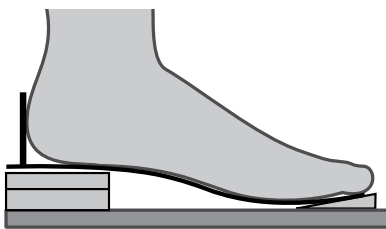

**Ankle Angle**

As Casted  Correct to: \_\_\_\_\_°

**Casting Block Setup**

Heel Height: \_\_\_\_\_ & Toe Ramp: \_\_\_\_\_

**Heel Wedge**

Attached  Unattached

Shoe Heel Height = \_\_\_\_\_

**Set Heel Wedge to:**

Calculate from Cast Block Setup

Set to SVA of: \_\_\_\_\_°

Other \_\_\_\_\_°

• **Calculated** = Casted Heel – Shoe Heel

• **SVA** = (Set AFO to SVA first) AFO Heel – Shoe Heel

• **Other** = Clinician Specified Amount

**SCAN INPUT REQUIREMENTS**

SCAN TYPE  Split/Inside Cast  Outside Cast (Preferred)

Positive Model:  Unmodified  Modified  Direct Patient

MEASUREMENTS Average Cast Thickness \_\_\_\_\_ mm

Outside Cast Forefoot ML \_\_\_\_\_ Outside Cast Ankle ML \_\_\_\_\_

**CLINICIAN:** \_\_\_\_\_ **PATIENT ID:** \_\_\_\_\_

**PREFERRED METHOD OF CONTACT**  CELL  TEXT  EMAIL  NG MOBILE \_\_\_\_\_

## DEVICE

**Options**

Single Upright  Double Upright  Hybrid

**Modifications**

**Standard**  Tone Reduction  ST Mod  
 Intrinsic Heel Mod \_\_\_\_\_ °  Medial  Lateral  
 Additional Build Ups/Reductions (detail in notes section)  
 Heel Height:  None  Other \_\_\_\_\_

**Corrected Ankle Position**

**Neutral**  As Is Other:  DF \_\_\_\_\_ °  PF \_\_\_\_\_ °

**Final Corrected Forefoot Position**

Right:  **Neutral**  As Is  Other \_\_\_\_\_  
 Left:  **Neutral**  As Is  Other \_\_\_\_\_

**Final Corrected Hindfoot Position**

Right:  **Neutral**  As Is  Other \_\_\_\_\_  
 Left:  **Neutral**  As Is  Other \_\_\_\_\_

## DESIGN

**Stirrup**

Soild  Solid-Extended  Solid-White  Split  UCBL  
 Other \_\_\_\_\_

**Ankle Joints**

DAAJ  Free Motion  Split  Limited Action  Dorsi Assist  
 Other \_\_\_\_\_

**Uprights Material**

AL  SS  TI

**Size**

1/4 x 3/4"  1/4 x 5/8"  3/16 x 1/2"  3/16 x 3/4"  
 3/16 x 5/8"  1/8 x 1/2"  Other \_\_\_\_\_

## DESIGN (continued)

**Pre-Set**

Pins  Springs  DF \_\_\_\_\_ °  PF \_\_\_\_\_ °

**Hybrid**

**Polypropylene**  Copolymer  Polyethylene  
 Other \_\_\_\_\_

**Thickness**

5/32"  1/4"  3/16"  1/8"

## FINISHING

**Straps**

Boot Hooks  Eyelets  T Strap  Medial  Lateral  
 Other \_\_\_\_\_

**Strap Material**

Leather  Dacron  Other \_\_\_\_\_

**Strap Color**

Black  White  Pink  Red  
 Beige  Green  Purple  Blue

**Shoes**

Heel Lift \_\_\_\_\_  
 Heel & Sole Lift \_\_\_\_\_  
 Medial Wedge \_\_\_\_\_  
 Lateral Wedge \_\_\_\_\_  
 Steel Shank \_\_\_\_\_  
 Other \_\_\_\_\_

**NOTES**

### TURNAROUND TIMES

To review current projected turnaround times for fabrication sites visit the [Daily HFN Capacity Webpage](#).